

FIG. 1

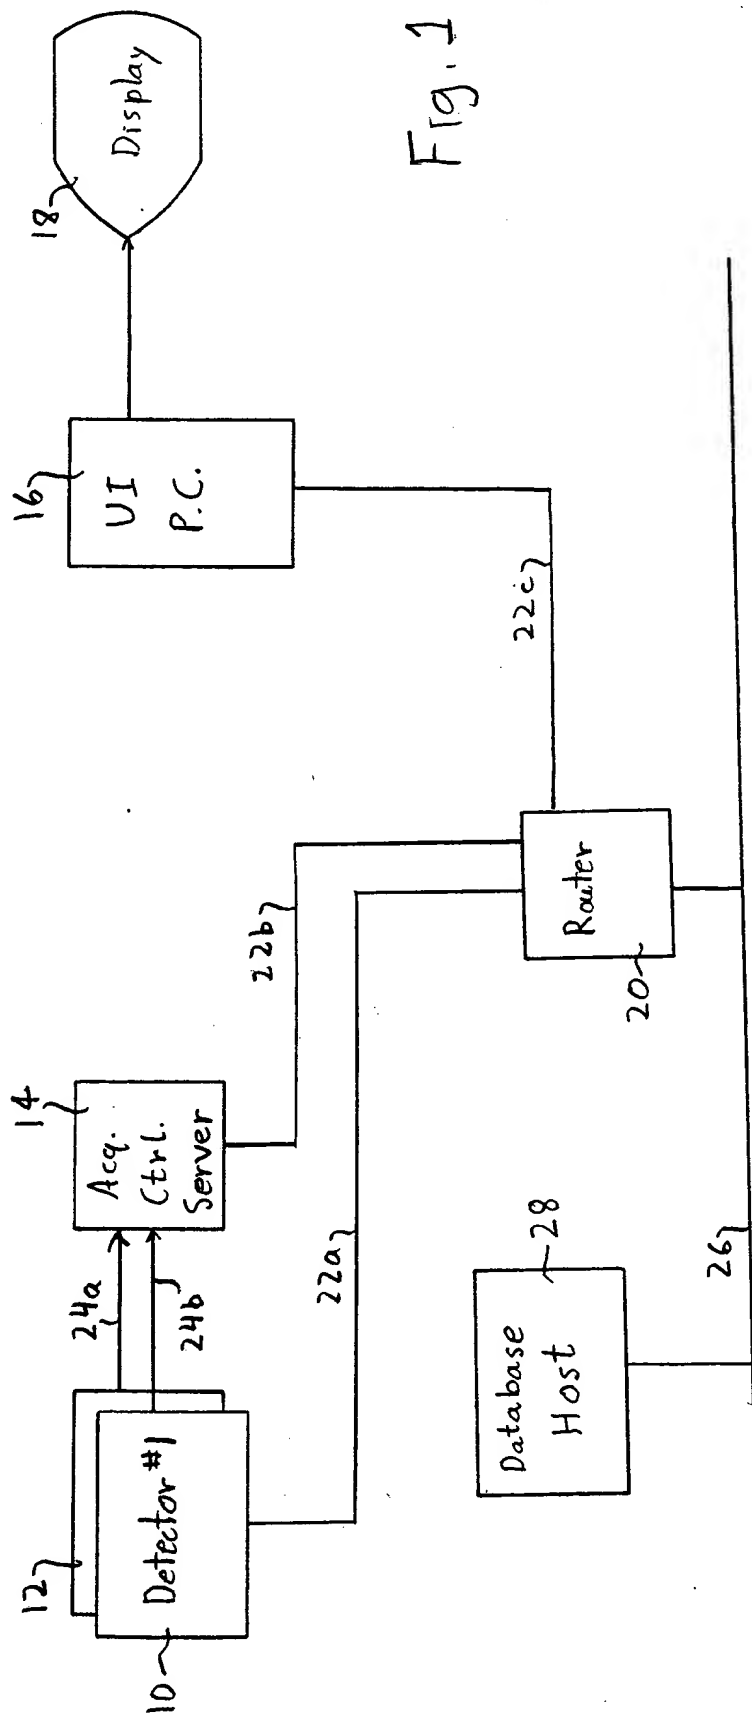


Fig. 1

FIG. 3

Procedure ID: Gated Spect ~ 300

Spect Parameters

Degrees in Orbit: 301
 Images in Orbit: 303
 Matrix Size: 305
 Starting Location: 307
 Rotation Direction: 309
 Orientation: 311
 Orbit (circular): 313
 Flood Correction: 315
 Acquisition Method: 317

Gated Parameters

No. of Gated Frames 331
 % R-R Interval Variance
 Max % Window 333
 Min % Window 335
 R-R Interval Fixed 337
 R-R Interval Vary 339
 No. Exclude After Variance 341
 Time Per ECT Azimuth or Total Beats 343

Time Avg R-R
 Frame No. Gated Frames
 Max Frame Max Frames
 Counts/Sec
 Beats 365

Processing
357

Isotope ID: 351
 Patient ID: 353
 View ID: 355

FIG. 3

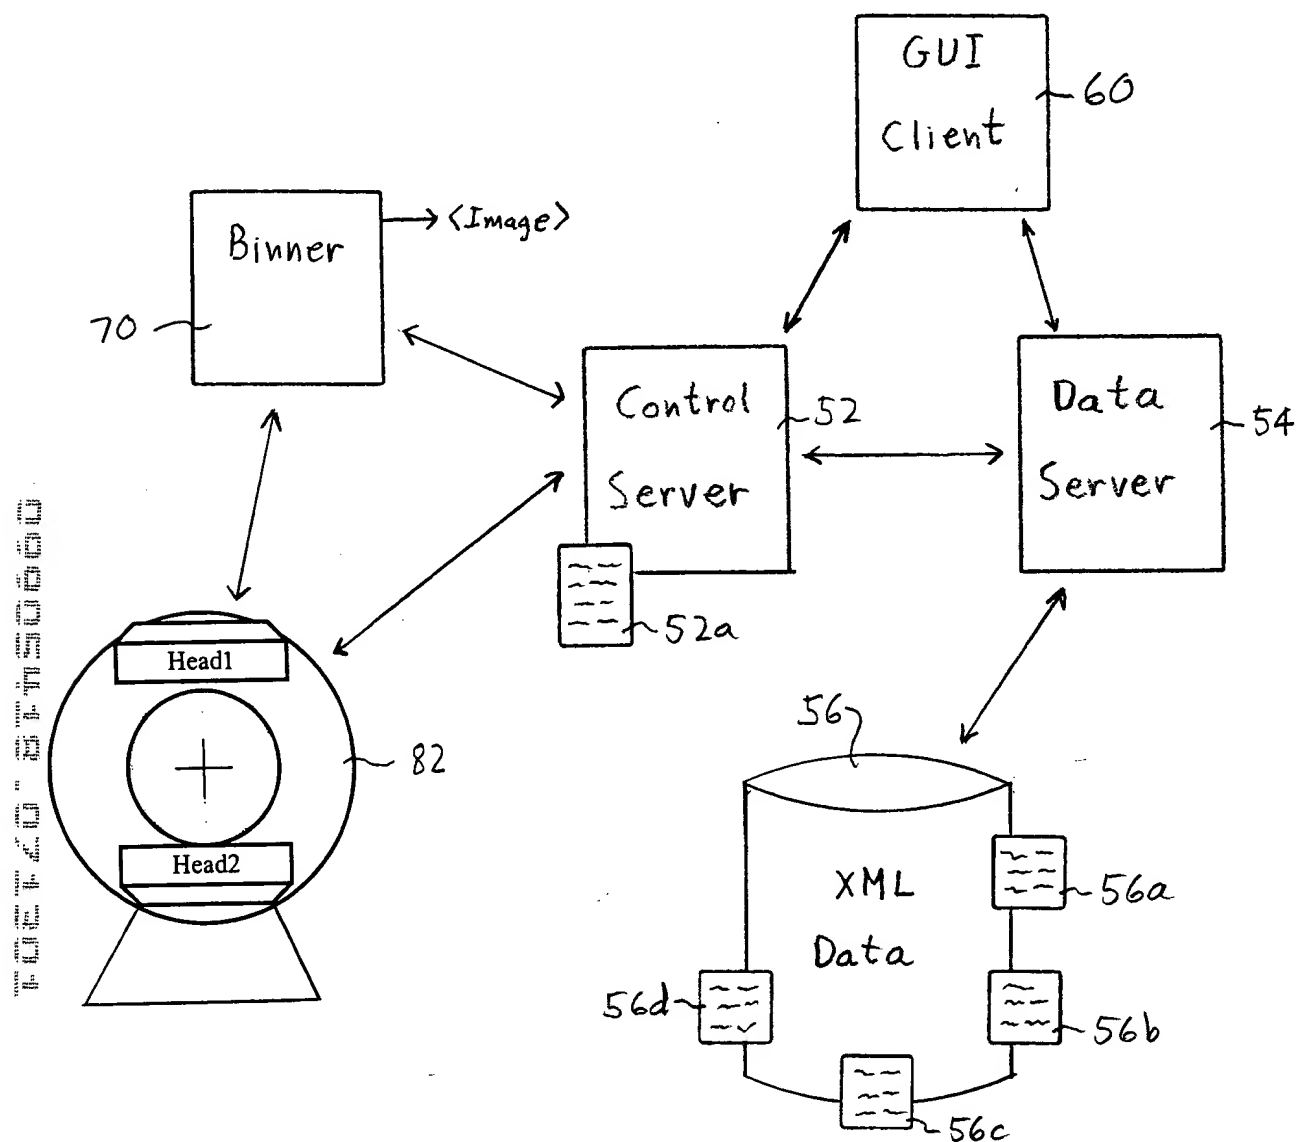
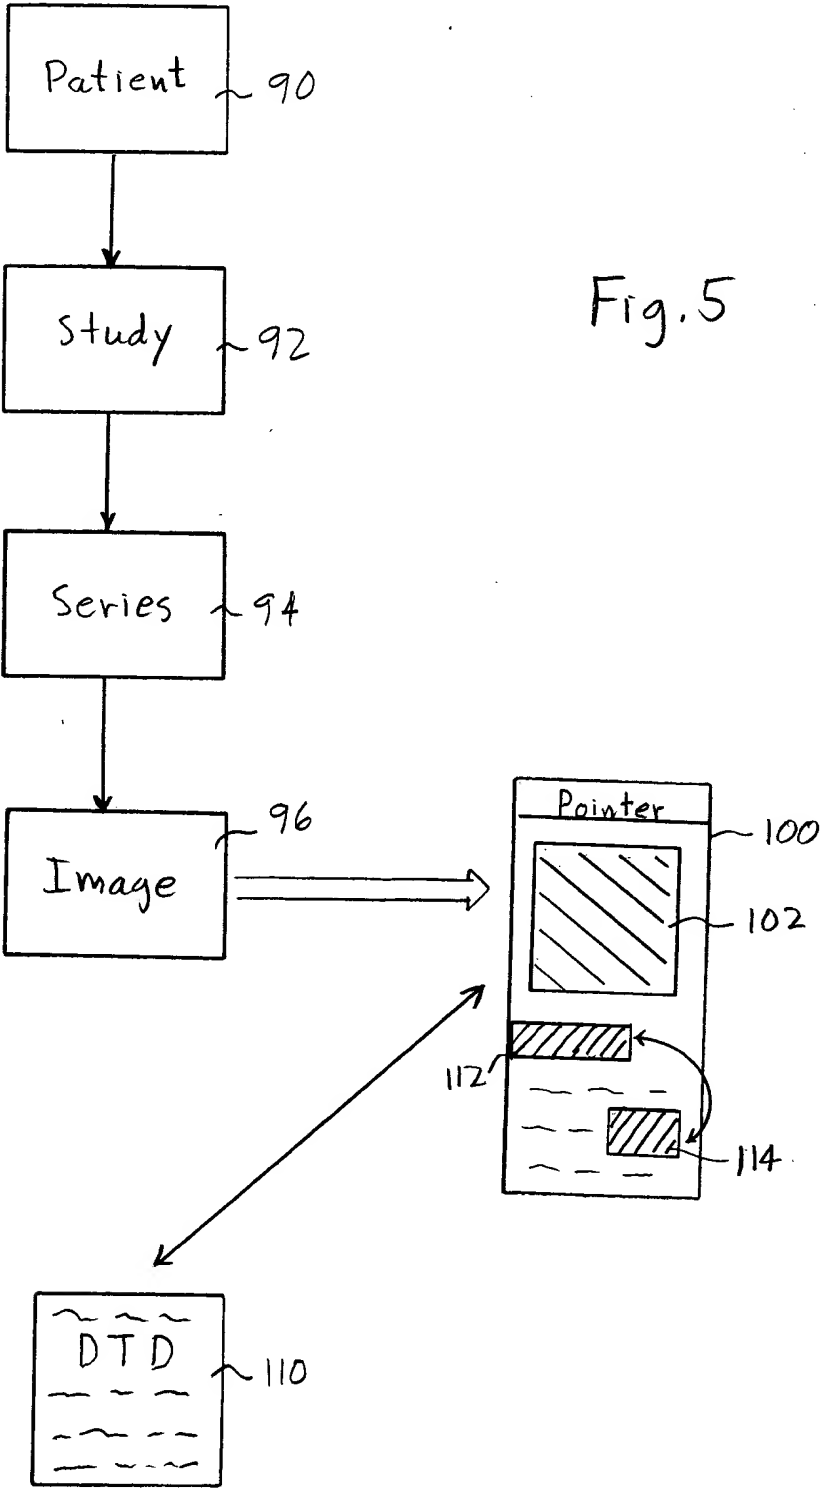
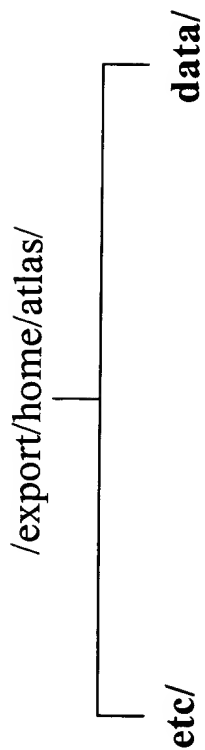
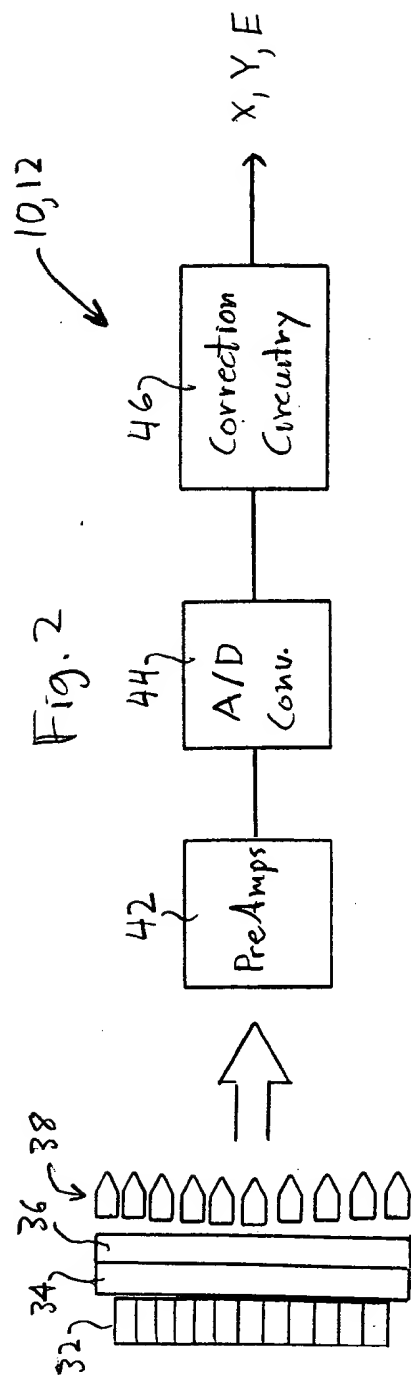


Fig. 4





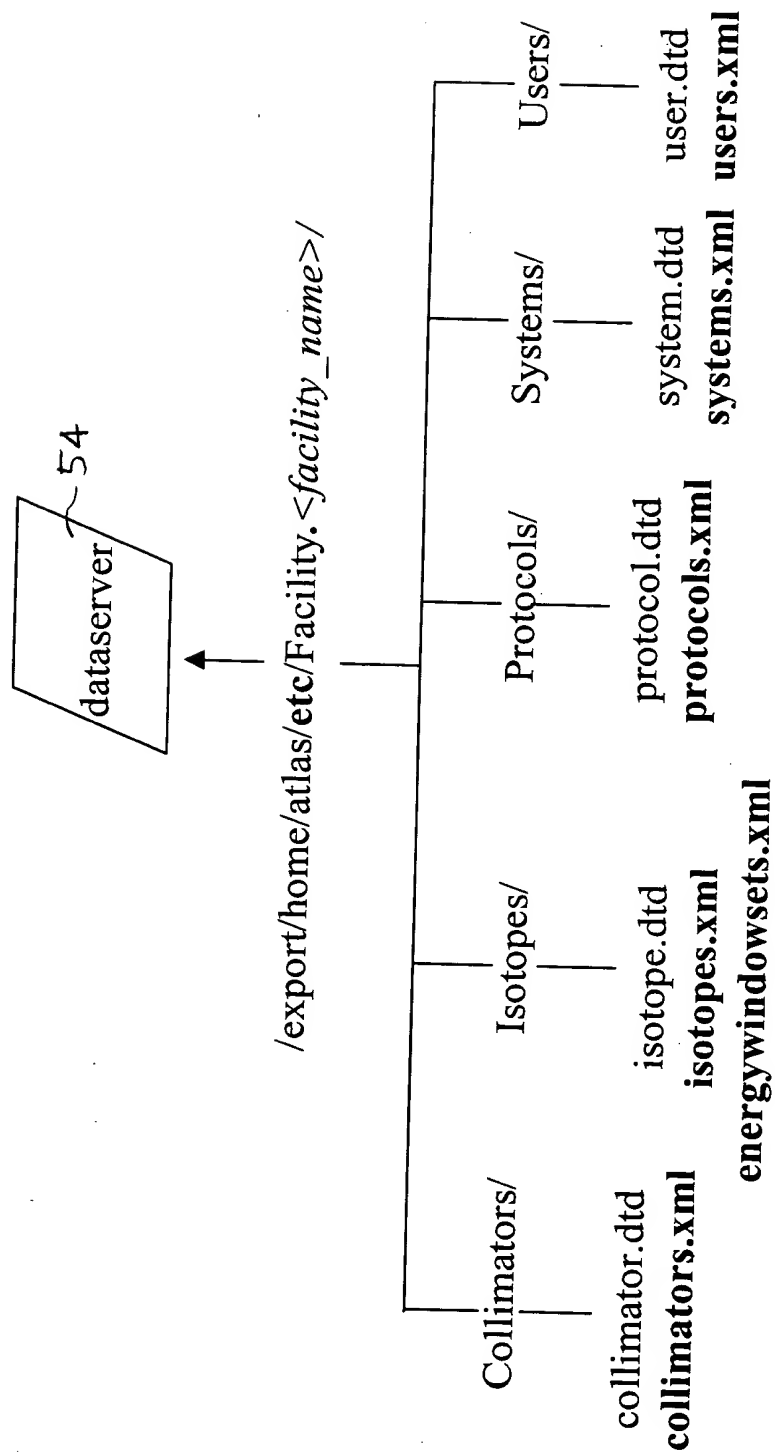


Fig. 7

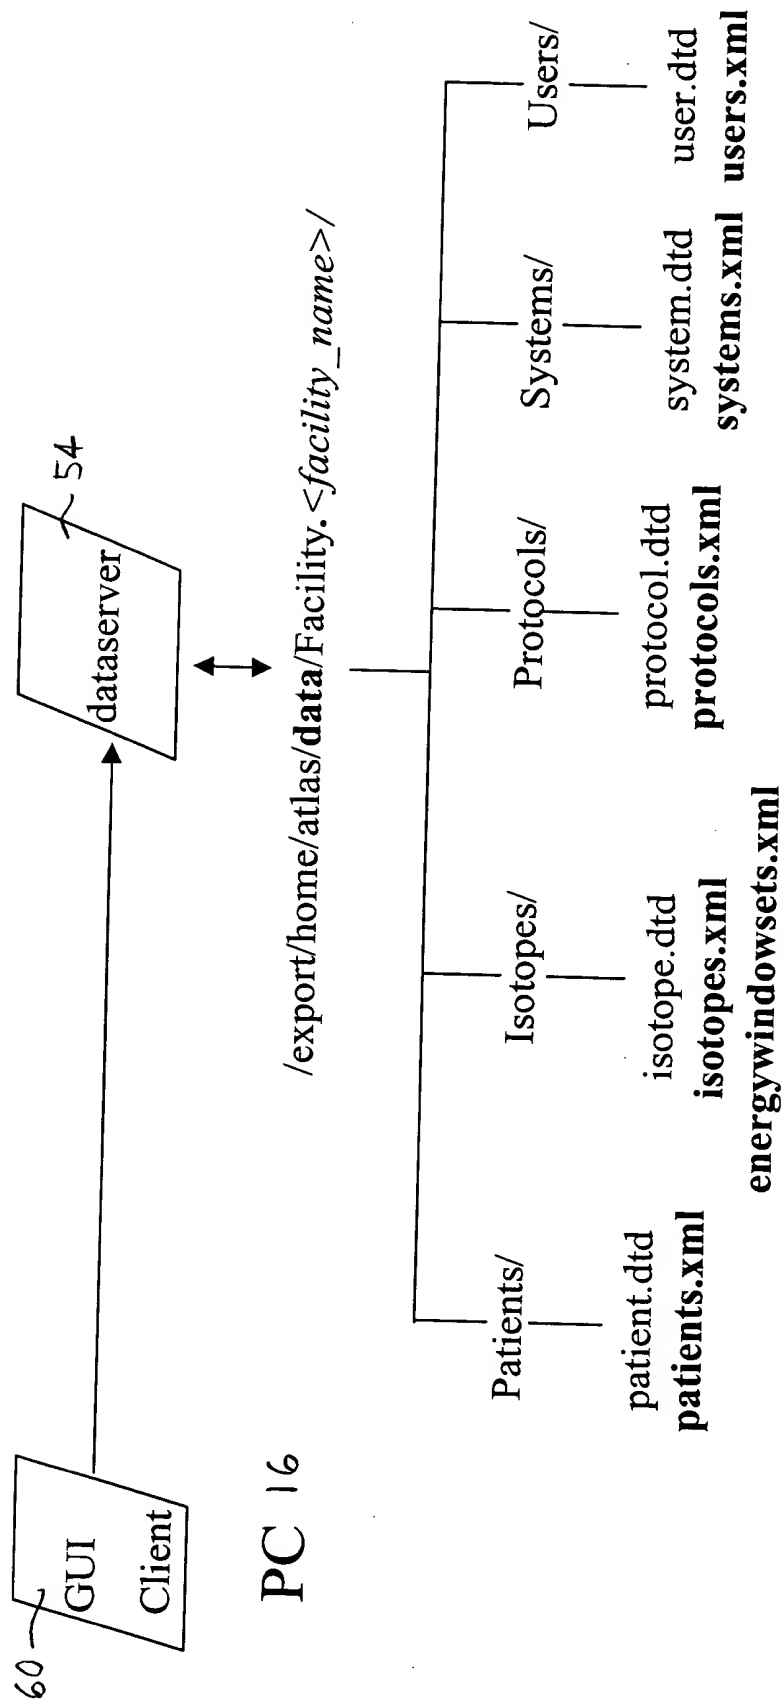


Fig. 8

FIG. 9

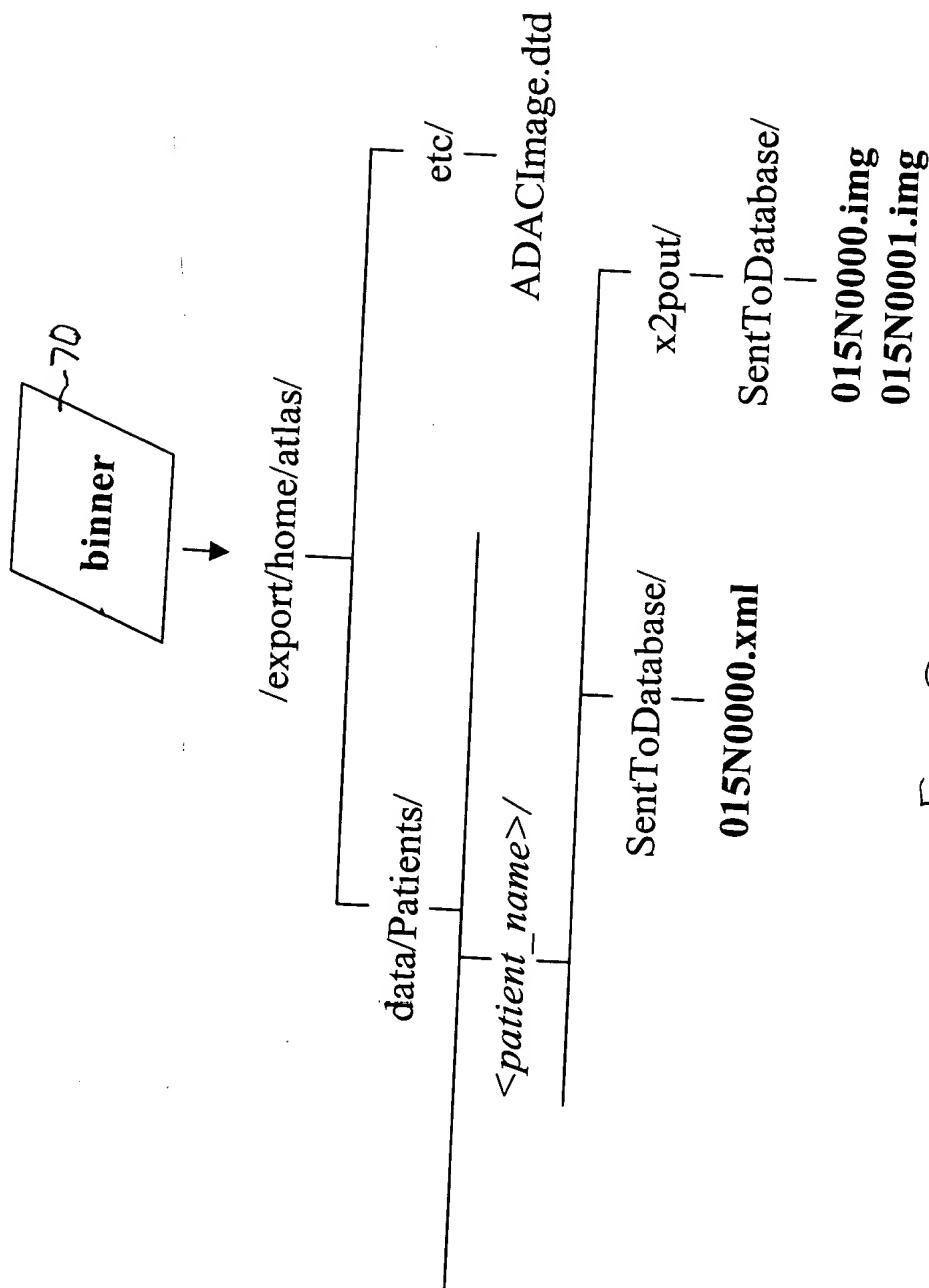


Fig. 9